

---

# User Manual for the *ML3 ThetaProbe*



**Eijkelkamp**  
Soil & Water

Nijverheidsstraat 9,  
6987 EN Giesbeek, The Netherlands

T +31 313 880 200  
E [info@eijkelkamp.com](mailto:info@eijkelkamp.com)  
I [www.eijkelkamp.com](http://www.eijkelkamp.com)

*Soil Moisture Sensor*

ML3-UM-2.1

M-14260702E

# Notices

## *Copyright*

All parts of the ML3 *ThetaProbe* design and documentation are the exclusive right of Delta-T Devices and covered under copyright law.

© 2017 Delta-T Devices Ltd

## *EMC Compliance*

See page 29.

## *Design changes*

Delta-T Devices Ltd reserves the right to change the designs and specifications of its products at any time without prior notice.

## *User Manual Version:*

ML3-UM-2.1 Jan 2017



Nijverheidsstraat 9,  
6987 EN Giesbeek, The Netherlands

**T** +31 313 880 200

**E** [info@eijkelkamp.com](mailto:info@eijkelkamp.com)

**I** [www.eijkelkamp.com](http://www.eijkelkamp.com)

# Contents

<b>Introduction</b>	<b>5</b>
<b>Description</b>	<b>5</b>
Features	5
Dimensions	6
<b>Parts list</b>	<b>7</b>
<b>Care and Safety</b>	<b>8</b>
<b>How the ML3 works</b>	<b>9</b>
<b>Operation</b>	<b>10</b>
<b>Cable Connections</b>	<b>10</b>
<b>Installation</b>	<b>11</b>
<b>Logger connections and configuration</b>	<b>12</b>
GP2	12
GP1	13
DL6	14
DL2e	15
Other data loggers	16
<b>HH2 Meter</b>	<b>17</b>
<b>Calibration</b>	<b>18</b>
Soil calibration	18
Sensor calibration	21
Soil moisture reading	22
<b>Troubleshooting</b>	<b>24</b>
<b>Technical Reference</b>	<b>26</b>
<b>Specifications</b>	<b>26</b>
Volumetric water content	26
Temperature	26
<b>Definitions</b>	<b>30</b>

<b>References</b>	<b>32</b>
<b>Technical Support</b>	<b>33</b>
<b>Appendix 1</b>	<b>35</b>
<b>Soil-specific Calibration</b>	<b>35</b>
<b>Laboratory calibration for non-clay soils</b>	<b>36</b>
<b>Laboratory calibration for clay soils</b>	<b>39</b>
<b>Appendix 2:</b>	<b>42</b>
<b>The ML3 Temperature Sensor</b>	<b>42</b>
ML3 Temperature Measurement	43
Effect of Temperature on Water Permittivity	44
Resistance to Temperature Lookup Table	45
<b>Index</b>	<b>46</b>

# Introduction

---

## Description

The *ML3* measures soil moisture content and temperature<sup>1</sup>. Its sealed plastic body is attached to four sensing rods which insert directly into the soil for taking readings.

A waterproof plug connects to a choice of signal cables. Both extension cables and extension tubes can be used.

The soil moisture output signal is a differential analogue DC voltage. This is converted to soil moisture by a data logger or meter using the supplied general soil calibrations.

It can also be calibrated for specific soils.

## Features

- Soil moisture accurate to  $\pm 1\%$
- Soil temperature to  $\pm 0.5^{\circ}\text{C}$  over  $0\text{-}40^{\circ}\text{C}$
- Low salinity sensitivity
- Excellent stability
- Minimal soil disturbance
- Easy installation at depth in augered holes
- Waterproof connector to IP68
- Rugged, weatherproof and can be buried.
- Good electrical immunity
- Choice of cabling system options
- Cable connector, cylindrical profile and extension tube design simplifies removal for servicing.

See also ***Specifications*** on page 26



---







<sup>1</sup> A data logger is required for temperature measurements


# Dimensions



# Parts list

Your shipment may include the following:

Part	Sales Code	Description
	<b>ML3</b>	ML3 sensor with Quick Start Guide
	<b>SMSC/d-HH2</b>	0.9m cable connects to HH2 meter via 25-way D-connector
	<b>SMSC/lw-05</b>	5m cable with 200mm flying leads for connecting to logger
	<b>EXT/5W-05</b> <b>EXT/5W-10</b> <b>EXT/5W-25</b>	5, 10 and 25m extension cables. IP68 M12 connectors
	<b>ML/EX50</b> <b>ML/EX100</b>	50 and 100cm Extension Tube
	<b>SM-AUG-100</b>	45mm spiral auger 1.2m long

	<p><b>ML3-Kit</b></p>	<p><b>ML3 sensor, HH2 meter, cable SMC/d-HH2, Insertion kit ML-INK1, 4 spare steel pins, spare battery, carry case HHCC3, HH2 manual, ML3 Quick Start</b></p>
--	-----------------------	---

## Care and Safety

- The rods of the ML3 are sharp in order to ease insertion. Care must be taken and handling precautions followed.
- Take care when attaching cables to ensure that the connectors are clean, undamaged and properly aligned *before* pushing the parts together.
- Do not pull the ML3 out of the soil by its cable.
- If you feel strong resistance when inserting the ML3 into soil, it is likely you have encountered a stone. Stop pushing and re-insert at a new location.
- Avoid touching the rods or exposing them to other sources of static damage, particularly when powered up.
- Keep the ML3 in its protective tube when not in use.

To prevent personal injury and damage to the probe always store and transport the ML3 in this protective tube

**CAUTION**  
**SHARP PINS**






# How the ML3 works



When power is applied to the ML3...



...it creates a 100MHz waveform (similar to FM radio).



The waveform is applied to an array of stainless steel rods which transmit an electromagnetic field into the soil.




The water content of the soil surrounding the rods...

$\epsilon$

...dominates its **permittivity**.

(A measure of a material's response to polarisation in an electromagnetic field. Water has a permittivity  $\approx 81$ , compared to soil  $\approx 4$  and air  $\approx 1$ )



The permittivity of the soil has a strong influence on the applied field...

$V_{out}$





...which is detected by the ML3, resulting in a stable voltage output that...

**Soil Moisture**  
22 %

...acts as a simple, sensitive measure of **soil moisture content**.

# Operation
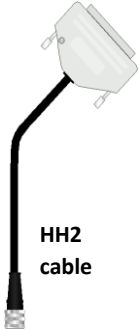
## Cable Connections

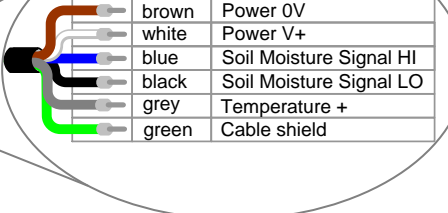 <p><b>HH2 cable</b></p>	 <p><b>Extension cables</b></p>	 <p><b>Logger cables</b></p>	 <table border="1"> <tbody> <tr> <td>brown</td> <td>Power 0V</td> </tr> <tr> <td>white</td> <td>Power V+</td> </tr> <tr> <td>blue</td> <td>Soil Moisture Signal HI</td> </tr> <tr> <td>black</td> <td>Soil Moisture Signal LO</td> </tr> <tr> <td>grey</td> <td>Temperature +</td> </tr> <tr> <td>green</td> <td>Cable shield</td> </tr> </tbody> </table>	brown	Power 0V	white	Power V+	blue	Soil Moisture Signal HI	black	Soil Moisture Signal LO	grey	Temperature +	green	Cable shield
brown	Power 0V														
white	Power V+														
blue	Soil Moisture Signal HI														
black	Soil Moisture Signal LO														
grey	Temperature +														
green	Cable shield														
0.9m	5m 10m 25m	5m with 200 mm bare leads													

- Take care when attaching cables to ensure that the connectors are clean, undamaged and properly aligned **before** pushing the parts together.
- Screw together firmly to ensure the connection is water-tight.
- Extension cables can be joined up to a recommended maximum of 100m – see Specifications on page 26

---

# Installation

## *Surface installation and spot measurements*

- Clear away any stones. Pre-form holes in very hard soils before insertion.
- Push the ML3 into the soil until the rods are fully inserted. Ensure good soil contact.
- If you feel strong resistance when inserting the ML3, you have probably hit a stone. Stop, and re-insert at a new location.



Note: The ML3 is not suitable for soil surface temperature measurements. For soil temperature near the surface dig a trench and install horizontally as shown below. Cover both ML3 and the first 30cm of cable with at least 5cm of soil.


## *Installing at depth*

- Make a 45mm diameter hole, preferably at about 10° to the vertical using the **SM-AUG-100** auger.
- Connect an extension tube e.g. **ML/EX50**
- Push the ML3 into the soil until rods are fully inserted. Ensure good soil contact.



## *Alternatively*

- Dig a trench, and install horizontally.

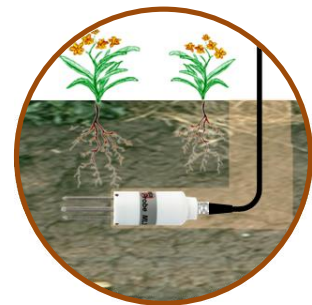

---

# Logger connections and configuration


## GP2

- 6 ML3s can connect to each GP2 wired as a differential, powered sensors.
- 12 ML3s can be connected if you do not use the temperature sensor. For this you will also need a 5 gland expansion lid GP2-G5-LID.



These details illustrate connection to Channels 1 and 2:

<i>ML3 wiring</i>	<i>Colour</i>	<i>GP2 terminal</i>
Power 0V and Thermistor LO	brown	<b>CH1 (PGND)</b>
Power V+	white	<b>CH1 (PWR)</b>
Soil Moisture Signal HI	blue	<b>CH1 (+)</b>
Soil Moisture Signal LO	black	<b>CH1 (-)</b>
Thermistor HI	grey	<b>CH2(+) and CH2(-)</b>
Cable shield	green	<b>CH1 (PGND)</b>

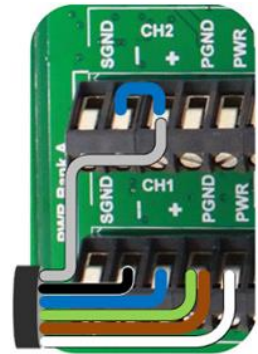

For configuration details see the **DeltaLINK 3<sup>2</sup>** software ML3 sensor **Info Panel, Help** or the **GP2 User Manual**.

Download the latest version of the DeltaLINK logger software from [www.delta-t.co.uk](http://www.delta-t.co.uk) or from our **Software and Manuals DVD**

---


<sup>2</sup> The GP2 logger needs the PC logger software DeltaLINK 3. This can be obtained from [www.delta-t.co.uk](http://www.delta-t.co.uk) or the **Software and Manuals DVD**.

# GP1

Two ML3s can connect to each GP1. Each ML3 is wired as a differential, powered sensor.

These details illustrate connection to Channels 1 and 3:

<i>ML3 wiring</i>	<i>Colour</i>	<i>GP1 terminal</i>
Power 0V and Thermistor LO	brown	<b>CH1 (GND) or Temp (GND)</b>
Power V+	white	<b>CH1 (PWR)</b>
Soil Moisture Signal HI	blue	<b>CH1 (+)</b>
Soil Moisture Signal LO	black	<b>CH1 (-)</b>
Temperature +	grey	<b>Temp3 (IN)</b>
Cable shield	green	<b>CH1 (GND)</b>

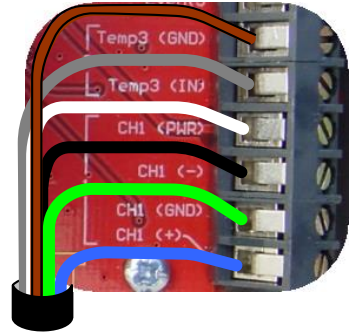

Using the DeltaLINK<sup>3</sup> logger software, configure channel 1 or 2 as sensor type **ML3** and channel 3 or 4 as an **ML3 Temperature** sensor. See also **GP1 Quick Start Guide** and the DeltaLINK on-line Help.

---

<sup>3</sup> The GP1 logger needs the PC logger software DeltaLINK version 3 or later. A free upgrade can be obtained from [www.delta-t.co.uk](http://www.delta-t.co.uk) or from the **Software and Manuals DVD**.


## DL6

6 ML3s can be connected to a DL6. Each ML3 is wired as a differential, powered sensor. A DL6 logger can only read one ML3 temperature sensor.



These details illustrate connection to channels 6 & 7:

<i>ML3 wiring</i>	<i>Colour</i>	<i>DL6 terminal</i>
Power 0V	brown	<b>0V</b>
Power V+	white	<b>V+</b>
Soil Moisture Signal HI	blue	<b>IN+</b>
Soil Moisture Signal LO	black	<b>IN-</b>
Temperature +	grey	<b>RES IN+</b>
Cable shield	green	<b>---</b>

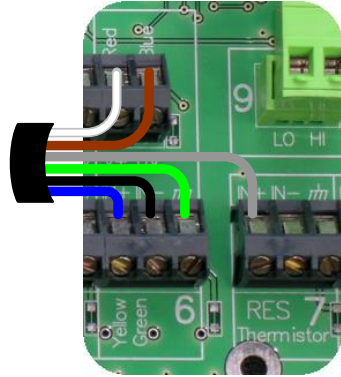

In DeltaLINK<sup>4</sup> configure channel 6 as type **ML3** and channel 7 as a type **ML3 Temperature** sensor.

See also the **DL6 Quick Start Guide** and the DeltaLINK online Help.

---

<sup>4</sup> The DL6 logger needs the PC logger software DeltaLINK version 3 or later. A free upgrade can be obtained from [www.delta-t.co.uk](http://www.delta-t.co.uk) or from the **Software and Manuals DVD**.

## DL2e

Up to 60 ML3s can be connected to a DL2e logger (if not using the temperature sensor channel).


Up to 30 ML3s can be connected if also reading the temperature sensor.

Each ML3 is connected as a differential, powered sensor.



These details illustrate connection to Channels 57 and 58 using a LAC1 input card configured in 15-channel mode, and warm-up channel 63:

<i>ML3 wiring</i>	<i>Colour</i>	<i>DL2e terminal</i>
Power 0V	brown	CH62- or 61-
Power V+	white	CH63 NO
Soil Moisture Signal HI	blue	CH58+
Soil Moisture Signal LO	black	CH58-
Temperature +	grey	CH57+ and CH57-
Cable shield	green	CH61- or 62-

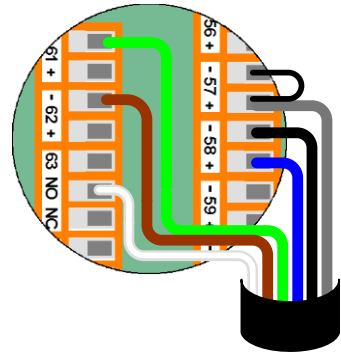

Configure the chosen DL2e logger channels by selecting the appropriate **S3M** and **S3O** sensor types for mineral and organic soils and **S3T** for the temperature sensor type listed in the Ls2Win<sup>5</sup> sensor library.

See the **DL2e User Manual** and the Ls2Win online help

---

<sup>5</sup> You need a PC running Ls2Win version 1.0 SR10 or later. A free upgrade can be obtained from [www.delta-t.co.uk](http://www.delta-t.co.uk) or from the **Software and Manuals DVD**.

## Other data loggers

- The ML3 should be connected as a differential, powered sensor.
- Configure the logger to convert the ML3 readings from milliVolts into soil moisture units by using either :-  
**Polynomial conversion** on page 22 or  
**Linearisation table** on page 23

Output signals in the range 0 to 1.0 volts from the ML3 correspond to a range of ~0 to 60% water content in mineral soils – see page 23.

Note: The ML3 has been optimised for warm-up of 0.5 to 1 second duration. It is recommended that the sensor is not powered continuously.

- The temperature sensor output should be read as a resistance and the logger configured with a look-up table to convert the measured resistance to temperature.

See **ML3 Temperature Measurement** on page 43

and **Resistance to Temperature Lookup Table** on page 45.



## HH2 Meter

You need version 2.7 or later for both the PC software **HH2Read** and the HH2 firmware (see foot of page).

- Connect the ML3 to the HH2 meter.
- Press **Esc** to turn the meter on, and if necessary press again until the HH2 displays the start-up screen.
- Set the meter to read from an ML3:
  - ▶ Press **Set** and scroll down to the **Device** option.
  - ▶ Press **Set** again and scroll down to select ML3.
  - ▶ Press **Set** to confirm this choice.



Device: ◀ ML3

- Make sure the HH2 is correctly configured for your soil type:
  - ▶ At the start-up screen, press **Set** and scroll down to the **Soil Type** option.
  - ▶ Press **Set** again and scroll down to the appropriate soil type (use **Mineral** for sand, silt or clay soils or **Organic** for peaty soils)
  - ▶ Press **Set** to confirm this choice.
- Choose the units you want for displaying readings.
  - ▶ At the start-up screen, press **Set** and scroll down to the **Display** option.
  - ▶ Press **Set** again and scroll down to select units.
  - ▶ Press **Set** to confirm this choice.

Soil Type:  
◀ Mineral

- Press **Read** to take a reading.
- Press **Store** to save or **Esc** to discard the reading.
- Remove the ML3 from the soil and move to a new location...
- If you have saved data, connect your HH2 to a PC and run **HH2Read** to retrieve the readings.

ML3 store?  
20.3%vol



See also: **Support for the ML3 Soil Moisture Sensor with an HH2** and **HH2 User Manual** and **HH2 User Manual Addendum to V4 - ML3**.

Note: the HH2 does not display or store ML3 temperature readings.

Note: For an upgrade contact Delta-T.


# Calibration

The ML3 is provided with general calibrations for **mineral** and **organic** soils which can be used to convert the output from the sensor directly into soil moisture when used with Delta-T loggers and the HH2 moisture meter. This section explains how these calibrations work, how to adapt them for other soils and how to provide calibrations for other data loggers.

The ML3 measures volumetric soil moisture  $\theta$ , by detecting the dielectric properties of the damp soil – the permittivity,  $\epsilon$ , or more conveniently the **refractive index**, which is closely equivalent to  $\sqrt{\epsilon}$ . The ML3 response is best understood in these stages:


## 1. Soil calibration

$$\theta \rightarrow \sqrt{\epsilon}$$

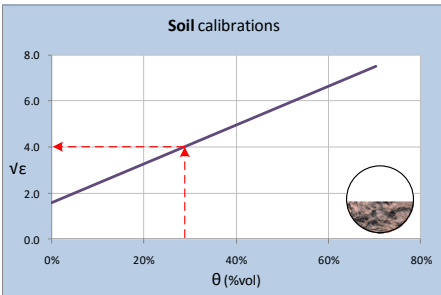


## 2. Sensor calibration

$$V \rightarrow \sqrt{\epsilon}$$

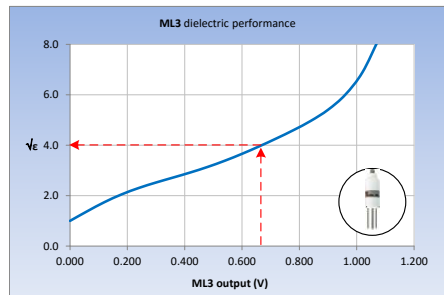

## 3. Soil moisture reading

$$V \rightarrow \theta$$

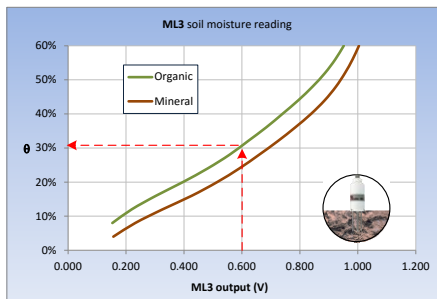


# Soil calibration

Damp soil is essentially a mixture of soil particles, air and water, and together these components determine its dielectric properties, including the refractive index  $\sqrt{\epsilon}$ . The refractive index of the mixture is approximated simply by adding the contributions from the individual components [ref 4].

For a particular soil, the contribution from the soil particles can be assumed to be constant, so the refractive index measured by the ML3 is only affected by changes to the water content,  $\theta$ . This relationship simplifies to:

$$\sqrt{\epsilon} = a_0 + a_1 \cdot \theta$$

where the coefficients  $a_0$  and  $a_1$  conveniently parameterise the dielectric properties of soils.

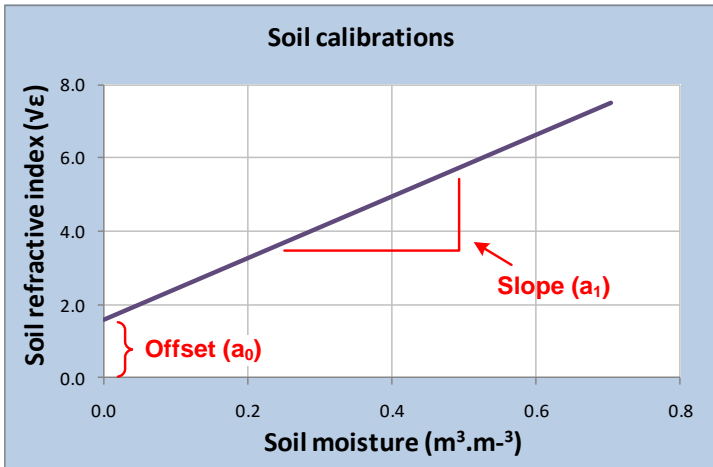

Note that:


$a_0 = \sqrt{\epsilon_{dry\_soil}}$  is usually between 1.3 to 2.3

$a_1$  corresponds approximately to  $\sqrt{\epsilon_{water}} - 1$  and usually takes a value about 8.0. Real soil values for  $a_0$  and  $a_1$  can vary significantly from these guidelines when they are affected by other factors – in particular, bound water in clay may result in higher values of  $a_1$ .

## General soil calibrations

Most soils can be characterised simply by choosing one of the two general calibrations we supply, one for mineral soils (predominantly sand, silt and clay) and one for organic soils (with a high organic matter content).

	$a_0$	$a_1$
Mineral soils	1.6	8.4
Organic soils	1.3	7.7

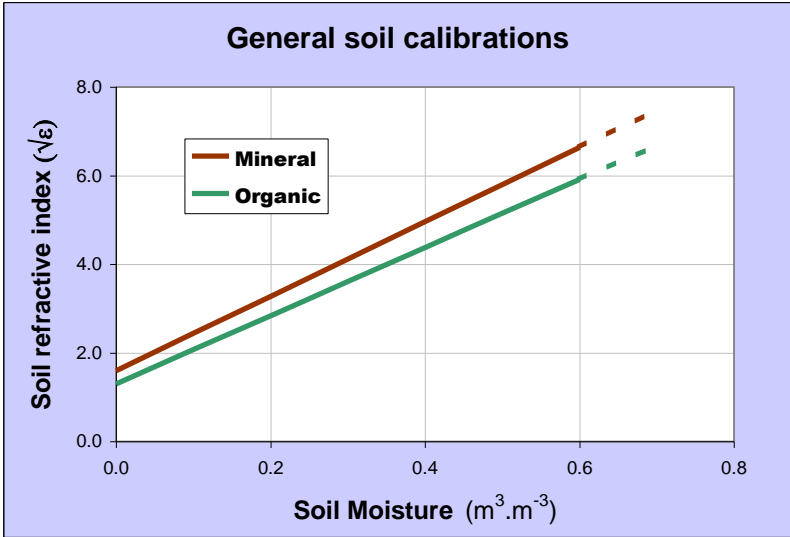

These values have been used to generate the polynomial conversions and linearisation tables in the **Soil moisture reading** section.


## Soil-specific calibration

Instead of adopting these general calibrations, you may wish to determine specific calibration values of  $a_0$  and  $a_1$  for your soil. This procedure is fairly straightforward if you can get access to standard laboratory equipment and is described in detail in Appendix 1 on page 34.

Soil specific calibration can significantly improve the accuracy of individual readings - but make less of an improvement to readings where installation and sampling errors are high.

## Sensor calibration

Each ML3 is individually adjusted to provide consistent dielectric performance:

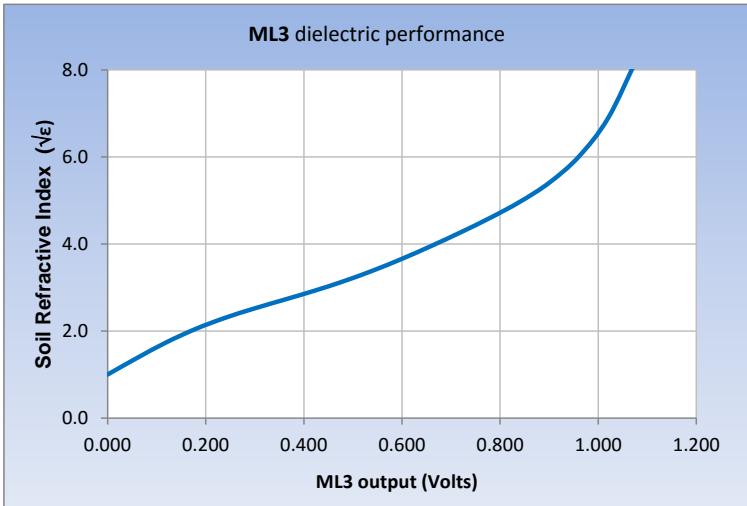

This response can be approximated either by a polynomial (below) or by a linearisation table (see page 23):

**Polynomial** (for use over the full range of ML3 readings)

$$\sqrt{\epsilon} = 1.0 + 6.175V + 6.303V^2 - 73.578V^3 + 183.44V^4 - 184.78V^5 + 68.017V^6$$

where  $V$  is the ML3 output in Volts

# Soil moisture reading

## Polynomial conversion

Combining the **Soil calibrations** and **Sensor calibration** steps, the conversion equation becomes:

$$\theta = \frac{[1.0 + 6.175V + 6.303V^2 - 73.578V^3 + 183.44V^4 - 184.78V^5 + 68.017V^6] - a_0}{a_1}$$

where  $a_0$  and  $a_1$  are the calibration coefficients.

For a generalised **mineral** soil this becomes:

$$\theta_{\text{mineral}} = -0.071 + 0.735V + 0.75V^2 - 8.759V^3 + 21.838V^4 - 21.998V^5 + 8.097V^6$$

And for a generalised **organic** soil:

$$\theta_{\text{organic}} = -0.039 + 0.802V + 0.819V^2 - 9.556V^3 + 23.823V^4 - 23.997V^5 + 8.833V^6$$

## Linearisation table

For use over the full range of ML3 readings

V	$\sqrt{\epsilon}$	V	$\sqrt{\epsilon}$	V	$\sqrt{\epsilon}$	V	$\sqrt{\epsilon}$	V	$\sqrt{\epsilon}$
0.000	1.000	0.240	2.305	0.480	3.139	0.720	4.269	0.960	6.001
0.060	1.381	0.300	2.521	0.540	3.385	0.780	4.601	1.020	6.890
0.120	1.741	0.360	2.719	0.600	3.659	0.840	4.966	1.080	8.282
0.180	2.050	0.420	2.920	0.660	3.955	0.900	5.406	1.140	10.531

## Linearisation table conversion

The conversion from ML3 reading (Volts) to soil moisture  $\theta$  ( $\text{m}^3.\text{m}^{-3}$  or %vol) can be accomplished by a look-up table.

The following table lists the values used for the DL2e data logger:

Soil moisture %vol	Mineral soil Volts	Organic soil Volts	Soil moisture %vol	Mineral soil Volts	Organic soil Volts
-4	-2.090	-2.090	52	0.956	0.887
0	0.096	0.048	56	0.982	0.922
4	0.156	0.097	60	1.004	0.951
8	0.232	0.153	64	1.023	0.976
12	0.326	0.220	68	1.040	0.997
16	0.427	0.304	72	1.054	1.016
20	0.514	0.396	76	1.068	1.032
24	0.591	0.482	80	1.080	1.046
28	0.659	0.557	84	1.091	1.059
32	0.724	0.620	88	1.101	1.071
36	0.783	0.683	92	1.110	1.082
40	0.838	0.740	96	1.119	1.092
44	0.886	0.795	100	1.127	1.101
48	0.924	0.844	104	2.090	2.090

# Troubleshooting

Always try to identify which part of the measurement system is the source of the difficulty. For the *ML3* this may fall into one of the following areas:

## *The measurement device*

What equipment is being used to read the probe output?

- A Delta-T HH2 Moisture Meter.  
Note: the HH2 does not measure ML3 temperature.
- A Delta-T data logger such as the GP1, GP2, DL6 or DL2e

## **Check Versions**

Check you have the correct versions:

HH2 Meter: Firmware version 2.7 and PC software HH2read version 2.7 or later are recommended.

GP1, GP2 & DL6 Loggers: DeltaLINK version 3.0 or later is required.

DL2e Logger: Ls2Win 1.0 SR10 is required

Consult the user manuals or the on-line help for these devices and their related software.

Try alternative types of equipment if you have them available.

Check that you are using an appropriate soil calibration and the correct conversion method – see **Calibration** section.

## *The ML3 itself*

Try to isolate the problem into one of the following areas

- The ML3 or the connecting cable

Then try to narrow down the area further

- Mechanical problems faults, or damage
- Electrical or electronic problems or faults



## Functional check

The following two simple checks can be used to establish whether your ML3 is functioning within expected bounds:

### Air reading

Hold the ML3 away from other objects and take a reading using an HH2 meter, or voltmeter or logger.

The reading should be  $0 \pm 4\text{mV}$  when used with a 5m cable.

### Warning : Do not touch the pins



### Mid range reading – dip rod tips in water

If you wish to take a quick reading to check the sensor is working you can dip the sensor into water.

With the pins half-immersed in tap water an HH2 should read over 1000 mV or, if set to read %vol and with soil type set to Organic, it should read in the range 80 to 100%vol.



# Technical Reference

## Specifications

Volumetric water content	
Accuracy	±1% vol over 0 to 50% vol and 0-40°C using soil specific calibrations
Measurement range	0 to 100% vol with reduced accuracy <sup>6</sup>
Salinity error (see p.27)	≤3.5%vol over 50 to 500 mS.m <sup>-1</sup> and 0-50% vol
Output Signal	0-1V differential ≈ 0 to 60% vol nominal
Output compatible with	GP1, GP2, DL6, DL2e, HH2
Temperature	
Sensor accuracy	±0.5°C over 0-40°C <i>not including logger or cabling error</i>
Output	Resistance <sup>7</sup> : 5.8kΩ to 28kΩ
Output compatible with	GP1, GP2, DL6 <sup>8</sup> , DL2e
Cabling error contribution (to temperature readings)	Negligible for GP1, GP2 & DL6 (any cable length) Negligible for DL2e (with 5m cable) <sup>9</sup>
Maximum cable length	100m (GP1, GP2 & DL6 data loggers) 100m (DL2e: water content measurement) 25m (DL2e: temperature measurement)
Power requirement	5-14VDC, 18mA for 0.5 to 1s
Operating range	-20 to +60°C
Environment	IP68
Sample volume	>95% influence within 40mm dia. cylinder 60mm long (approx. 75 cm <sup>3</sup> ) around central rod.
Dimensions/weight	170.5 mm x 39.8 mm dia./138 gm (without cable)

6 In water (no soil present) the reading may not be 100% vol. It depends on a0 and a1 but can still be used as a quick check that the unit is working. See page 25.



7 See Appendix 2 on page 42.

8 Note: The DL6 has only one temperature channel. The DL6 error contribution to ML3 temperature measurement is negligible compared to the accuracy of the ML3 temperature sensor itself. The two only become comparable below -15C.

9 DL2e logger users can apply a correction in the Ls2Win logging software (for cable lengths >5m)

## Conductivity response

This chart shows how salinity affects the output of the soil moisture sensor at various soil moisture levels.

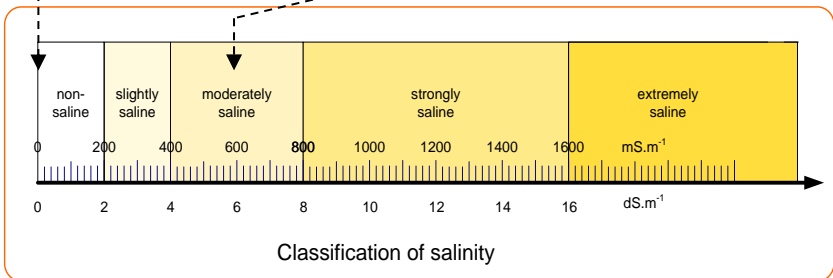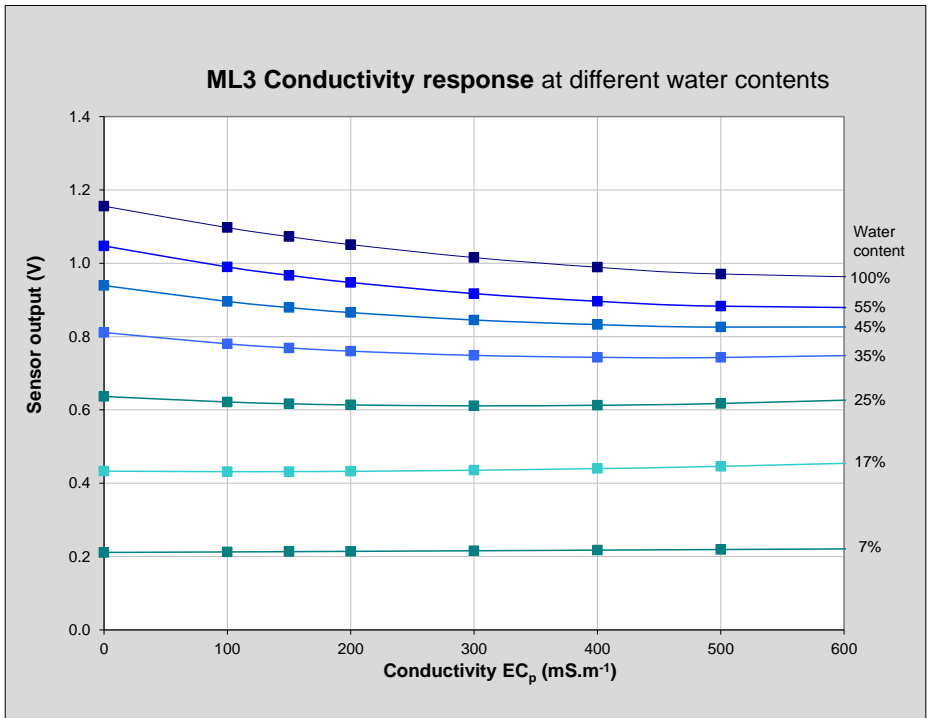


## Temperature response of soil moisture readings

The effect of temperature on the ML3 soil moisture readings in any particular soil will depend on a combination of effects:

- The ML3 soil moisture electronics has very low temperature sensitivity, and makes a negligible contribution to the overall sensitivity.
- The refractive index of water ( $\sqrt{\epsilon}$ , see **Calibration** section) reduces as the temperature increases. This produces a negative temperature response particularly in soils or substrates with high water content.
- Water that is bound to the surface of soil particles has a much lower refractive index than free water. The percentage of bound water decreases with temperature and this produces a positive temperature response particularly in clay soils at lower water contents.

The last two effects partially offset each other, but in soil conditions where one or the other effect dominates, the ML3 will appear to have a significant temperature response. This illustration is based on the model in reference 7, see page 32.

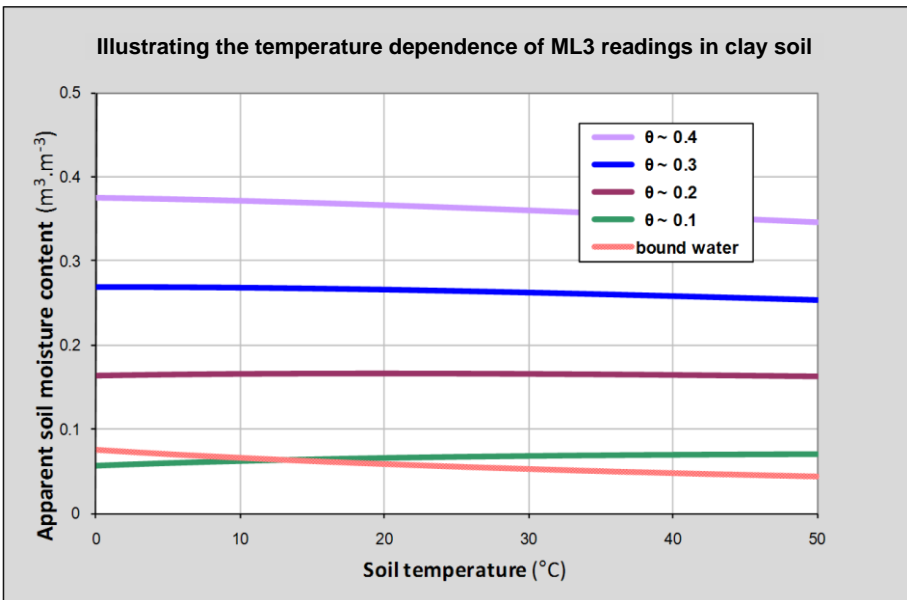

---

*Note: ice has a quite different refractive index from water, so ML3 soil moisture readings cannot be interpreted reliably when inserted into soil below 0°C.*

---

## ***Electromagnetic Compatibility (EMC)***

### **General information**

ML3 is a Class A product, intended for operation in non-residential environments.

Only use cables and accessories authorised by Delta-T (sensor cables from other sources for example may adversely affect product performance and affect quality of results).

If possible route cables along the soil surface or bury them – this also reduces possible trip hazard and animal damage.

Do not modify the product or its supplied accessories.

See also ***ML3 EMC Guidance*** on the Software and Manuals DVD Issue 3.

### **Regulatory information**

#### **Europe**

This device conforms to the essential requirements of the EMC directive 2004/108/EC, based on the following test standards:

EN61326-1:2006 Electrical requirement for measurement, control and laboratory use. EMC requirements: Group 1, Class A equipment – (emissions section only).

EN61326-1:2006 Electrical requirement for measurement, control and laboratory use. EMC requirements: Basic Immunity (immunity section only).

#### **FCC compliance (USA)**

This device conforms to Part 18 of FCC rules – Industrial, Scientific & Medical Equipment.

Note: with reference to FCC Part 18.115 Elimination and investigation of harmful interference.

(a) The operator of the ISM equipment that causes harmful interference to radio services shall promptly take appropriate measures to correct the problem.

---

# Definitions

**Volumetric Soil Moisture Content** is defined as

$$\theta_V = \frac{V_W}{V_S} \quad \begin{array}{l} \text{where } V_W \text{ is the volume of water contained in the} \\ \text{sample and} \\ V_S \text{ is the total volume of the soil sample.} \end{array}$$

The preferred units for this ratio are  $\text{m}^3 \cdot \text{m}^{-3}$ , though %vol is frequently used.

Soil Moisture Content varies from approx.  $0.02 \text{ m}^3 \cdot \text{m}^{-3}$  for sandy soils at the permanent wilting point, through approx.  $0.4 \text{ m}^3 \cdot \text{m}^{-3}$  for clay soils at their field capacity, up to values as high as  $0.85 \text{ m}^3 \cdot \text{m}^{-3}$  in saturated peat soils.

**Gravimetric Soil Moisture Content** is defined as

$$\theta_G = \frac{M_W}{M_S} \text{ g} \cdot \text{g}^{-1} \quad \begin{array}{l} \text{where } M_W \text{ is the mass of water in the sample,} \\ \text{and } M_S \text{ is the total mass of the dry sample.} \end{array}$$

To convert from volumetric to gravimetric water content, use the equation

$$\theta_G = \theta_V \times \frac{\rho_W}{\rho_S} \quad \begin{array}{l} \text{where } \rho_W \text{ is the density of water } (= 1 \text{ g} \cdot \text{cm}^{-3}), \\ \text{and } \rho_S \text{ is the bulk density of the sample } \left( \frac{M_S}{V_S} \right). \end{array}$$

## Organic and Mineral soil definitions:

The general calibrations have been optimised to cover a wide range of soil types, based on the following definitions:

Soil type	optimised around organic content:	use for organic contents:	bulk density range: (g.cm <sup>-3</sup> )	use for bulk densities: (g.cm <sup>-3</sup> )
<b>Mineral</b>	~ 1 %C*	< 7 %C	1.25 - 1.5	> 1.0
<b>Organic</b>	~ 40 %C	> 7 %C	0.2 - 0.7	< 1.0

\* Note: %C denotes "percentage Carbon" and is a measure of organic content


## Salinity

The preferred SI units for ionic conductivity are **mS.m<sup>-1</sup>** (where S is Siemens, the unit of electric conductance = ohm<sup>-1</sup>).

The following conversions apply:

$$\begin{aligned}
 1 \text{ mS.m}^{-1} &= 0.01 \text{ dS.m}^{-1} \\
 &= 0.01 \text{ mS.cm}^{-1} \\
 &= 10 \text{ } \mu\text{S.cm}^{-1}
 \end{aligned}$$

Soil salinity can be classified using the following descriptive categories:

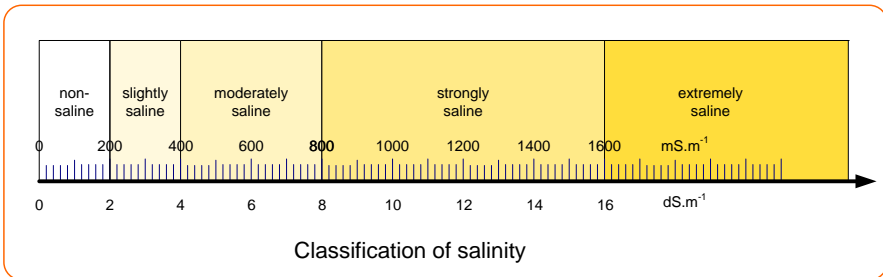

See also [http://www.land.vic.gov.au/DPI/Vro/vrosite.nsf/pages/water\\_spotting\\_soil\\_salting\\_class\\_ranges#s1](http://www.land.vic.gov.au/DPI/Vro/vrosite.nsf/pages/water_spotting_soil_salting_class_ranges#s1)

# References

1. Gaskin, G.J. and J.D. Miller, 1996  
Measurement of soil water content using a simplified impedance measuring technique.  
*J. Agr. Engng Res* **63**, 153-160
2. Topp, G.C., J. L. Davis and A. P Annan 1980  
Electromagnetic determination of soil water content.  
*Water Resour. Res* **16**(3) 574-582
3. Whalley, W.R. 1993  
Considerations on the use of time-domain reflectometry (TDR) for measuring soil moisture content.  
*Journal of Soil Sci.* **44**, 1-9
4. White, I., J.H. Knight, S.J. Zegelin, and Topp, G.C. 1994  
Comments on 'Considerations on the use of time-domain reflectometry (TDR) for measuring soil water content' by W R Whalley  
*Journal of Soil Sci.* **45**, 503-508
5. Roth, C.H., M.A. Malicki, and R. Plagge, 1992  
Empirical evaluation of the relationship between soil dielectric constant and volumetric water content as the basis for calibrating soil moisture measurements.  
*Journal of Soil Sci.* **43**, 1-13
6. Knight, J.H. 1992  
Sensitivity of Time Domain Reflectometry measurements to lateral variations in soil water content.  
*Water Resour. Res.*, **28**, 2345-2352
7. Or, D. and J.M. Wraith 1999  
Temperature effects on soil bulk dielectric permittivity measured by time domain reflectometry: A physical model.  
*Water Resour Res.*, **35**, 371-383



# Technical Support

## *Terms and Conditions of Sale*

Our Conditions of Sale (ref: COND: 1/07) set out Delta-T's legal obligations on these matters. The following paragraphs summarise Delta T's position but reference should always be made to the exact terms of our Conditions of Sale, which will prevail over the following explanation.

Delta-T warrants that the goods will be free from defects arising out of the materials used or poor workmanship for a period of two years from the date of delivery.

Delta-T shall be under no liability in respect of any defect arising from fair wear and tear, and the warranty does not cover damage through misuse or inexpert servicing, or other circumstances beyond their control.

If the buyer experiences problems with the goods they shall notify Delta-T (or Delta-T's local distributor) as soon as they become aware of such problem.

Delta-T may rectify the problem by replacing faulty parts free of charge, or by repairing the goods free of charge at Delta-T's premises in the UK during the warranty period.

If Delta-T requires that goods under warranty be returned to them from overseas for repair, Delta-T shall not be liable for the cost of carriage or for customs clearance in respect of such goods. However, Delta-T requires that such returns are discussed with them in advance and may at their discretion waive these charges.

Delta-T shall not be liable to supply products free of charge or repair any goods where the products or goods in question have been discontinued or have become obsolete, although Delta-T will endeavour to remedy the buyer's problem.

Delta-T shall not be liable to the buyer for any consequential loss, damage or compensation whatsoever (whether caused by the negligence of the Delta-T, their employees or distributors or otherwise) which arise from the supply of the goods and/or services, or their use or resale by the buyer.

Delta-T shall not be liable to the buyer by reason of any delay or failure to perform their obligations in relation to the goods and/or services if the delay or failure was due to any cause beyond the Delta-T's reasonable control.

## **Extended Warranty**

All Delta-T Devices products have a two year (24 month) warranty as standard, but the ML3, SM150T and SM300 soil moisture sensors benefit from a 5 year warranty (60 months from date of delivery). Simply register the product(s) with us via [www.delta-t.co.uk](http://www.delta-t.co.uk) and we will add 3 more years to the standard warranty, extending it to the full 5 years duration. To qualify, products must be registered within 12 weeks of delivery.

All SM150s, SM150Ts, SM300s and ML3s sold since 1 January 2016 are eligible.

Visit the Support Section of our website [www.delta-t.co.uk](http://www.delta-t.co.uk) to register your sensor for an extended 5 year warranty.

## ***Service, Repairs and Spares***

Users in countries that have a Delta-T distributor or technical representative should contact them in the first instance.

Spare parts for our own instruments can be supplied and can normally be despatched within a few working days of receiving an order.

Spare parts and accessories for products not manufactured by Delta-T may have to be obtained from our supplier, and a certain amount of additional delay is inevitable.

No goods or equipment should be returned to Delta-T without first obtaining the return authorisation from Delta-T or our distributor.

On receipt of the goods at Delta-T you will be given a reference number. Always refer to this reference number in any subsequent correspondence. The goods will be inspected and you will be informed of the likely cost and delay.

We normally expect to complete repairs within one or two weeks of receiving the equipment. However, if the equipment has to be forwarded to our original supplier for specialist repairs or recalibration, additional delays of a few weeks may be expected. For contact details see below.

## ***Technical Support***

Users in countries that have a Delta-T distributor or technical representative should contact them in the first instance.

Technical Support is available on Delta-T products and systems. Your initial enquiry will be acknowledged immediately with a reference number. Make sure to quote the reference number subsequently so that we can easily trace any earlier correspondence.

In your enquiry, always quote instrument serial numbers, software version numbers, and the approximate date and source of purchase where these are relevant.

## ***Contact details:***

**Eijkelkamp**

***Soil & Water***

Nijverheidsstraat 9,  
6987 EN Giesbeek, The Netherlands

**T** +31 313 880 200

**E** info@eijkelkamp.com

**I** www.eijkelkamp.com

# Appendix 1

## Soil-specific Calibration

This note provides details of 2 techniques for generating soil-specific calibrations:


Laboratory calibration for substrates\* and non-clay soils

Laboratory calibration for clay soils

\* *We use the term substrate to refer to any artificial growing medium.*

### Underlying principle

Soil moisture content ( $\theta$ ) is proportional to the refractive index of the soil ( $\sqrt{\epsilon}$ ) as measured by the ML3 (see **Calibration** section).

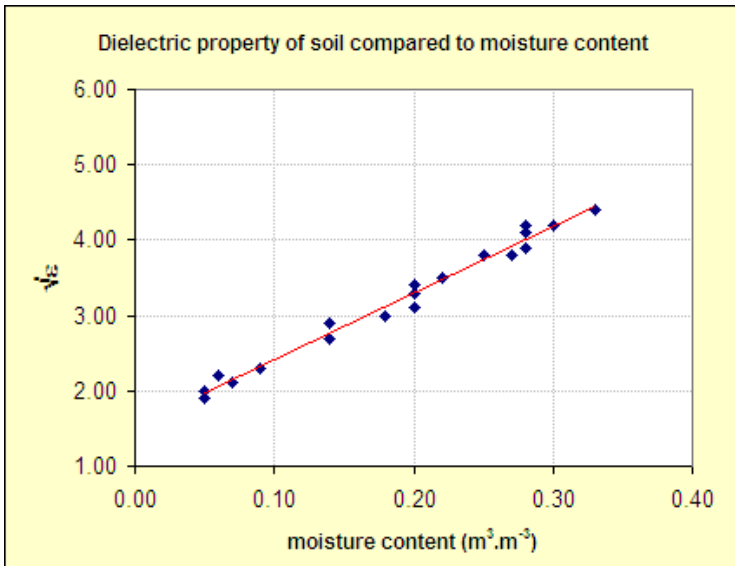

The goal of calibration is to generate two coefficients ( $a_0$ ,  $a_1$ ) which can be used in a linear equation to convert probe readings into soil moisture:




$$\sqrt{\epsilon} = a_0 + a_1 \times \theta$$





# Laboratory calibration for non-clay soils

This is the easiest technique, but it's not suitable for soils that shrink or become very hard when dry.

Equipment you will need:

- ML3 and meter
- Soil corer (if doing a calibration for a cohesive soil rather than sand or a substrate)
- Heat-resistant beaker ( $\geq 0.5$  litre)
- Weighing balance (accurate to  $< 1$ g)
- Temperature controlled oven (for mineral soils or substrates)

Process	Notes and example
	<p>Collect a damp sample of the soil or substrate.</p> <p>This sample needs to be unchanged from its in-situ density, to be <math>\geq 0.4</math> litre, to have the correct dimensions to fit the beaker, and to be generally uniform in water content.</p> <p>For cohesive soils this is most easily done with a soil-corer.</p> <p>Sandy soils can be poured into the beaker, but you should take the subsequent measurements immediately, as the water will quickly begin to drain to the bottom of the beaker.</p> <p>Compressible soils and composts often require measurement of the in-situ density and then need to be carefully reconstituted at that density within the beaker.</p>
	<p>Measure the volume occupied by the sample.</p> <p><b><math>L_s = 463.5\text{ml}</math></b></p>
	<p>Weigh the sample, including the beaker.</p> <p><b><math>W_w = 743.3\text{g}</math></b></p>

	<p>Insert ML3 into the sample and record its output in Volts.</p> <p><b><math>V_w = 0.572 V</math></b></p>
	<p>Dry the sample thoroughly.</p> <p>With mineral soils this is usually achieved by keeping it in the oven at 105°C for several hours or days (the time required depends on the sample size and porosity).</p> <p>For organic soils and composts it's usual to air-dry the sample to avoid burning off any volatile fractions.</p>
	<p>Weigh the dry sample in the beaker.</p> <p><b><math>W_0 = 627.2g</math></b></p>
	<p>Re-insert the ML3 into the dry sample and record this reading.</p> <p><b><math>V_0 = 0.089 V</math></b></p>
<p><b>Calculate <math>\alpha_0</math></b></p>	<p>For the ML3,</p> <p>In the dry soil <math>V = V_0 = 0.089</math> Volts</p> <p>Substitute this into the equation</p> $\sqrt{\epsilon} = 1.0 + 6.175V + 6.303V^2 - 73.578V^3 + 183.44V^4 - 184.78V^5 + 68.017V^6$ <p>gives <math>\sqrt{\epsilon_0} = 1.56</math></p> <p>Since <math>\theta_0 = 0</math>, this is the value needed for <math>\alpha_0</math></p> <p><b><math>\alpha_0 = 1.56</math></b></p>
<p><b>Calculate <math>\theta_w</math></b></p>	<p>The water content of the wet soil, <math>\theta_w</math>, can be calculated from the weight of water lost during drying, <math>(W_w - W_0)</math> and its volume, <math>L_s</math>:</p>

	$\theta_w = (W_w - W_0)/L_s = (743.3 - 627.2)/463.5 = 0.25$ $\theta_w = 0.25$
Calculate $a_1$	<p>In the wet soil <math>V = V_w = 0.572</math> Volts and substituting gives</p> $\sqrt{\varepsilon_w} = 3.53$ <p>Finally</p> $a_1 = (\sqrt{\varepsilon_w} - \sqrt{\varepsilon_0})/(\theta_w - \theta_0) = (3.53 - 1.56)/(0.25 - 0) = 7.87$ $a_1 = 7.87$
<b>Result</b>	$a_0 = 1.56$ $a_1 = 7.87$

In this example this soil is now calibrated.

You can now use these two numbers in place of the standard mineral or organic calibration factors to convert ML3 readings into volumetric water content  $\theta$  using:

$$\sqrt{\varepsilon} = a_0 + a_1 \times \theta$$




See also **Underlying principle** on page 35


# Laboratory calibration for clay soils

This technique is adapted to avoid the near-impossibility of inserting the ML3 into completely dry clay soil. It requires taking measurements at 2 significantly different, but still damp, moisture levels.


Equipment you will need:

- ML3 and meter
- Soil corer
- Heat-resistant beaker ( $\geq 500\text{ml}$ )
- Weighing balance (accurate to  $< 1\text{g}$ )
- Temperature controlled oven


<i>Process</i>	<i>Notes and example</i>
	<p>Collect a <u>wet</u> sample of the clay soil: 25 to 30% water content would be ideal.</p> <p>This sample needs to be unchanged from its in-situ density, to be <math>\geq 400\text{ml}</math>, to have the correct dimensions to fit the beaker, and to be generally uniform in water content.</p> <p>This is most easily done with soil-corer.</p>
	<p>Measure the volume occupied by the sample.</p> <p><b><math>L_s = 463.5\text{ml}</math></b></p>
	<p>Weigh the wet sample, including the beaker.</p> <p><b><math>W_w = 743.3\text{g}</math></b></p>




Insert ML3 into the wet sample and record its output in Volts.  
 **$V_w = 0.572 V$**




Dry the sample until still moist, ~15% water content. Gentle warming can be used to accelerate the process, but take care not to over-dry in places, and allow time for the water content to equilibrate throughout the sample before taking a reading.




Reweigh.  
 **$W_m = 693.2 g$**



Re-measure with the ML3.  
 **$V_m = 0.348 V$**



Dry the sample thoroughly.  
With clay soils this is usually achieved by keeping it in the oven at 105°C for several hours or days (the time required depends on the sample size and porosity).



Weigh the dry sample in the beaker.  
 **$W_o = 627.2 g$**

### Calculations

Substituting in the ML3 equation



	$\sqrt{\epsilon} = 1.0 + 6.175V + 6.303V^2 - 73.578V^3 + 183.44V^4 - 184.78V^5 + 68.017V^6$ <p>provides two dielectric values, <math>\sqrt{\epsilon_w}</math> and <math>\sqrt{\epsilon_m}</math>, at two known water contents, <math>\theta_w</math> and <math>\theta_m</math></p>
For the wet soil	Substituting $V_w = 0.572$ gives $\sqrt{\epsilon} = 3.53 = a_0 + a_1\theta$ for $\theta_w = (743.3 - 627.2)/463.5 = 0.25$
For the moist soil	Substituting $V_m = 0.348$ gives $\sqrt{\epsilon} = 2.68 = a_0 + a_1\theta_m$ For $\theta_m = (693.2 - 627.2)/463.5 = 0.14$
Calculate $a_1$	Then $a_1 = (\sqrt{\epsilon_w} - \sqrt{\epsilon_m})/(\theta_w - \theta_m) = 7.86$ <b><math>a_1 = 7.86</math></b>
Calculate $a_0$	and $a_0 = \sqrt{\epsilon_w} - (a_1 \cdot \theta_w) = 1.56$ <b><math>a_0 = 1.56</math></b>
<b>Result</b>	<b><math>a_1 = 7.86</math></b> <b><math>a_0 = 1.56</math></b>

In this example this soil is now calibrated.

You can now use these two numbers in place of the standard mineral or organic calibration factors to convert ML3 readings into volumetric water content  $\theta$  using:

$$\sqrt{\epsilon} = a_0 + a_1 \times \theta$$

See also page [Underlying principle](#) on page 35

# Appendix 2:

---

## The ML3 Temperature Sensor

Soil moisture content is used with the measurement of soil temperature in several major application areas including the following:

### Global warming and climate studies

Soils contain more than four times as much carbon as the CO<sub>2</sub> in the atmosphere, and each year they release about ten times as much carbon through soil respiration as the combined release through burning fossil fuels. Soil respiration rates are particularly sensitive to changes in both temperature and the moisture content of the soil.

Soils also have a significant interaction with climate as they store and release heat – soil temperature provides a measure of the energy partitioning, which in turn is strongly influenced by the effect of soil moisture on thermal conductivity.

### Civil engineering

Most civil engineering projects depend critically on the mechanical properties of soils. Those properties are effected by many different parameters, but moisture content and temperature are the two variables that are most likely to change over time, so may be measured together in order to assess their impact.

### Soil contamination and hydrogeology

Soil moisture is the main determinant for the movement of contaminants and solutes through soils, but temperature also has a significant influence so they are often measured together.

### Agriculture

Temperature may be measured alongside soil water content for studies of evapotranspiration, soil water balance and irrigation. Soil strength and seedling emergence depend on soil moisture and temperature, and both need to be taken into account when deciding when to sow.

## ML3 Temperature Measurement

The ML3 Temperature sensor uses a thermistor with a 10K resistance at 25 °C. However:

- A. This sensor has a different response curve from the more widely used 10K3A1B type. The response curve is given in the Resistance to Temperature Lookup Table on page 45.
- B. The Thermistor circuit shares the Power 0V wire. If the thermistor is measured when the ML3 is powered, the measured resistance measurement may need to be corrected for 18 mA ML3 supply current.

### GP2, GP1 and DL6 loggers

The 'ML3 Temperature' sensor type in DeltaLINK 3 performs the supply current correction.

### DL2e Logger

The linearization table for the 'S3T' sensor code ('ML3 Temperature') provides supply current correction for the **SMSC/lw-05** 5m logger cable ONLY.

### Extension cables and other cable lengths

Create your own custom sensor type(s) and linearization tables as described in Ls2Win Help topic, How to... 'Add or modify a sensor type in the sensor library'.

Enter corrected resistance values (R) for each linearization table point:

$$R = R5 + (0.059 \times Lex) \text{ k}\Omega \quad (\text{See footnote}^{10})$$

$$\text{or} \quad R = R5 + (0.9 \times Rc - 0.297) \text{ k}\Omega$$

where

R5 = value supplied in the table for the 'ML3 Temp, 5m' sensor type.

Lex = length of extension cable, excluding the 5m of **SMSC/lw-05** cable.

Rc = total cable resistance, including resistance of **SMSC/lw-05** cable, if fitted.

---

<sup>10</sup> Note: This equation only applies to Delta-T ML3 cables

## Other loggers

If your logger can be programmed so that the soil moisture and temperature readings can be taken sequentially (i.e. the sensor is not powered during the temperature reading), then the temperature can be obtained directly from the response curve on page 45.

Otherwise, correct the resistance reading before applying the response curve.

You need to know the resistance of the Power 0V wire in the ML3 cable ( $R_c$ ) and establish whether your logger uses voltage or current excitation for resistance measurement.

## Voltage Excited

You need to know the excitation voltage ( $V_{ref}$ ), reference resistance ( $R_{ref}$ ).

The correct resistance is given by the equation:

$$R = a_0 + a_1 * R_{meas}$$

Where:

$$a_0 = - I_c.R_c.R_{ref} / V_{ref}$$

$$a_1 = 1 - I_c.R_c / V_{ref}$$

$$I_c = 18 \text{ mA (ML3 sensor supply current)}$$

For Delta-T **EXT/5W-xx** series cables:

$$R_c = 0.066 \Omega.m^{-1}$$

For the **SMSC/lw-05** 5m logger cable

$$R_c = 0.33 \Omega$$

## Current Excited

You need to know the excitation current ( $I_{ex}$ ).

The corrected resistance is given by the equation (using terms defined above):


$$R = R_{meas} - I_c.R_c/I_{ex}$$

## Effect of Temperature on Water Permittivity

See **Temperature response of soil moisture readings** on page 28

# Resistance to Temperature Lookup Table

Temperature degrees C	Resistance Kohms
-25	90.538
-22	77.683
-19	66.854
-16	57.713
-13	49.968
-10	43.379
-7	37.759
-4	32.957
-1	28.844
2	25.299
5	22.244
8	19.608
11	17.321
14	15.334
17	13.606
20	12.098
23	10.780
26	9.623
29	8.611
32	7.720
35	6.935
38	6.241
41	5.627
44	5.080
47	4.595
50	4.162
53	3.775
56	3.430
59	3.121
62	2.843
65	2.593

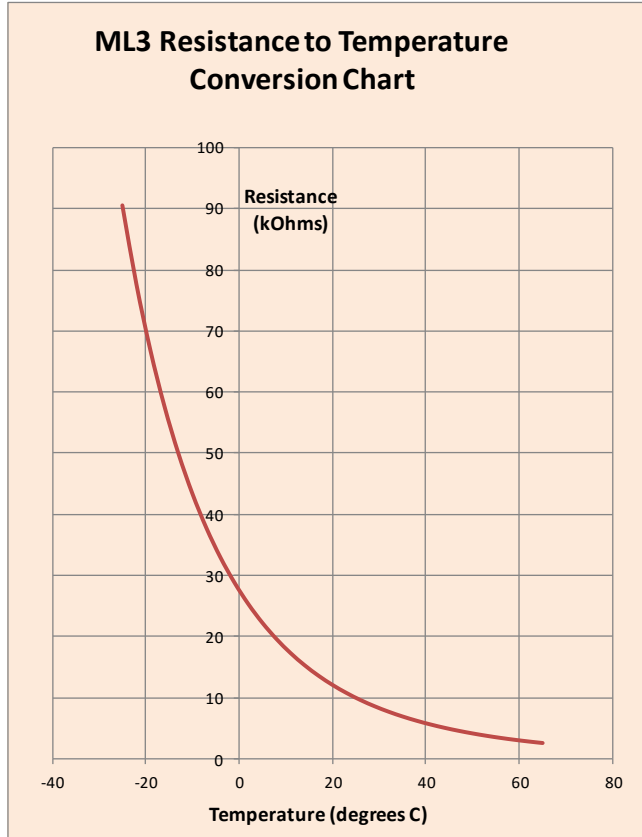

Note: This table has been optimised for use as a look-up table.

To minimise linear interpolation errors the data points fall either side of the manufacturers' specified sensor response curve. This helps optimise the overall accuracy of readings.

# Index

## A

**Agriculture**, 42  
Air reading, 25  
Auger, 7

## C

Cable Connections, 10  
Cable length correction, 43  
Calibration  
    check, 25  
    generalised, 22  
    sensor, 21, 22  
    soil, 19, 22  
    Soil, 35  
    soil-specific, 35  
Care and safety, 8  
Care and Safety, 8  
Certification  
    emc, 29  
**Civil engineering**, 42  
**climate**, 42  
Conductivity response, 27  
Connections, 12  
**contamination**, 42  
Conversions  
    linearisation table, 20, 21  
    polynomial, 20, 21  
Copyright, 2

## D

Data logger, 16, 23, 24, 25  
    DL2e, 23, 24  
    DL6, 24  
    GP1, 14, 24  
    other, 16  
Definitions, 30  
Description, 5

Dielectric  
    performance, 21  
    refractive index, 18, 19, 35  
Dimensions, 6  
DL6, 14

## E

EMC, 29  
Extension cables, 10

## F

FCC compliance, 29  
Features, 5

## G

**Global warming**, 42  
GP1, 13, 14, 24  
GP2, 12

## H

HH2, 7, 17, 18, 24, 25  
**hydrogeology**, 42

## I

Installation  
    buried, 11  
    insertion rod, 11  
    surface, 11

## L

Linearisation table, 23  
    volts to %vol, 23

## M

Meter, 24

Moisture content, 5, 9, 32, 35

## O

**Organic and Mineral**, 31

## P

Parts, 7

Permittivity, 9, 18, 32

Polynomial conversion, 22

## R

References, 32

Regulatory information, 29

Rods, 8, 9, 11

## S

**Sales code**, 7

Salinity, 31

Servicing, 34

**SMSC/lw-05**, 43

Soil

clay, 19, 20, 30, 35, 36, 39

mineral, 18, 20, 22, 36, 37, 40

organic, 18, 20, 22, 31, 37

stony, 11

soil calibrations, 20

Specifications, 2, 26

## T

Technical support, 33, 34

Temperature

    cable length correction, 43

Temperature response of soil moisture  
    readings, 28

Temperature sensor cable length  
    correction, 44

Temperature Sensor Lookup Table, 45

Troubleshooting, 24

## V

**Volumetric Soil Moisture**, 30

## W

Warning

    Care and Safety, 8

Warning, 25